
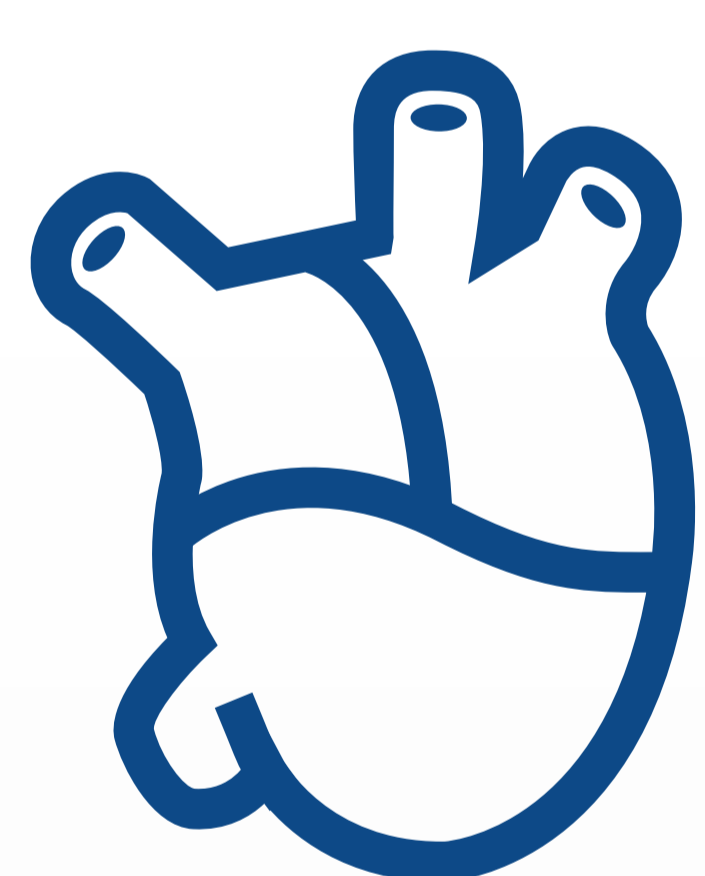


# Medtronic


## EVOLUT™ PRO+ TAVI SYSTEM

### EXPECT MORE

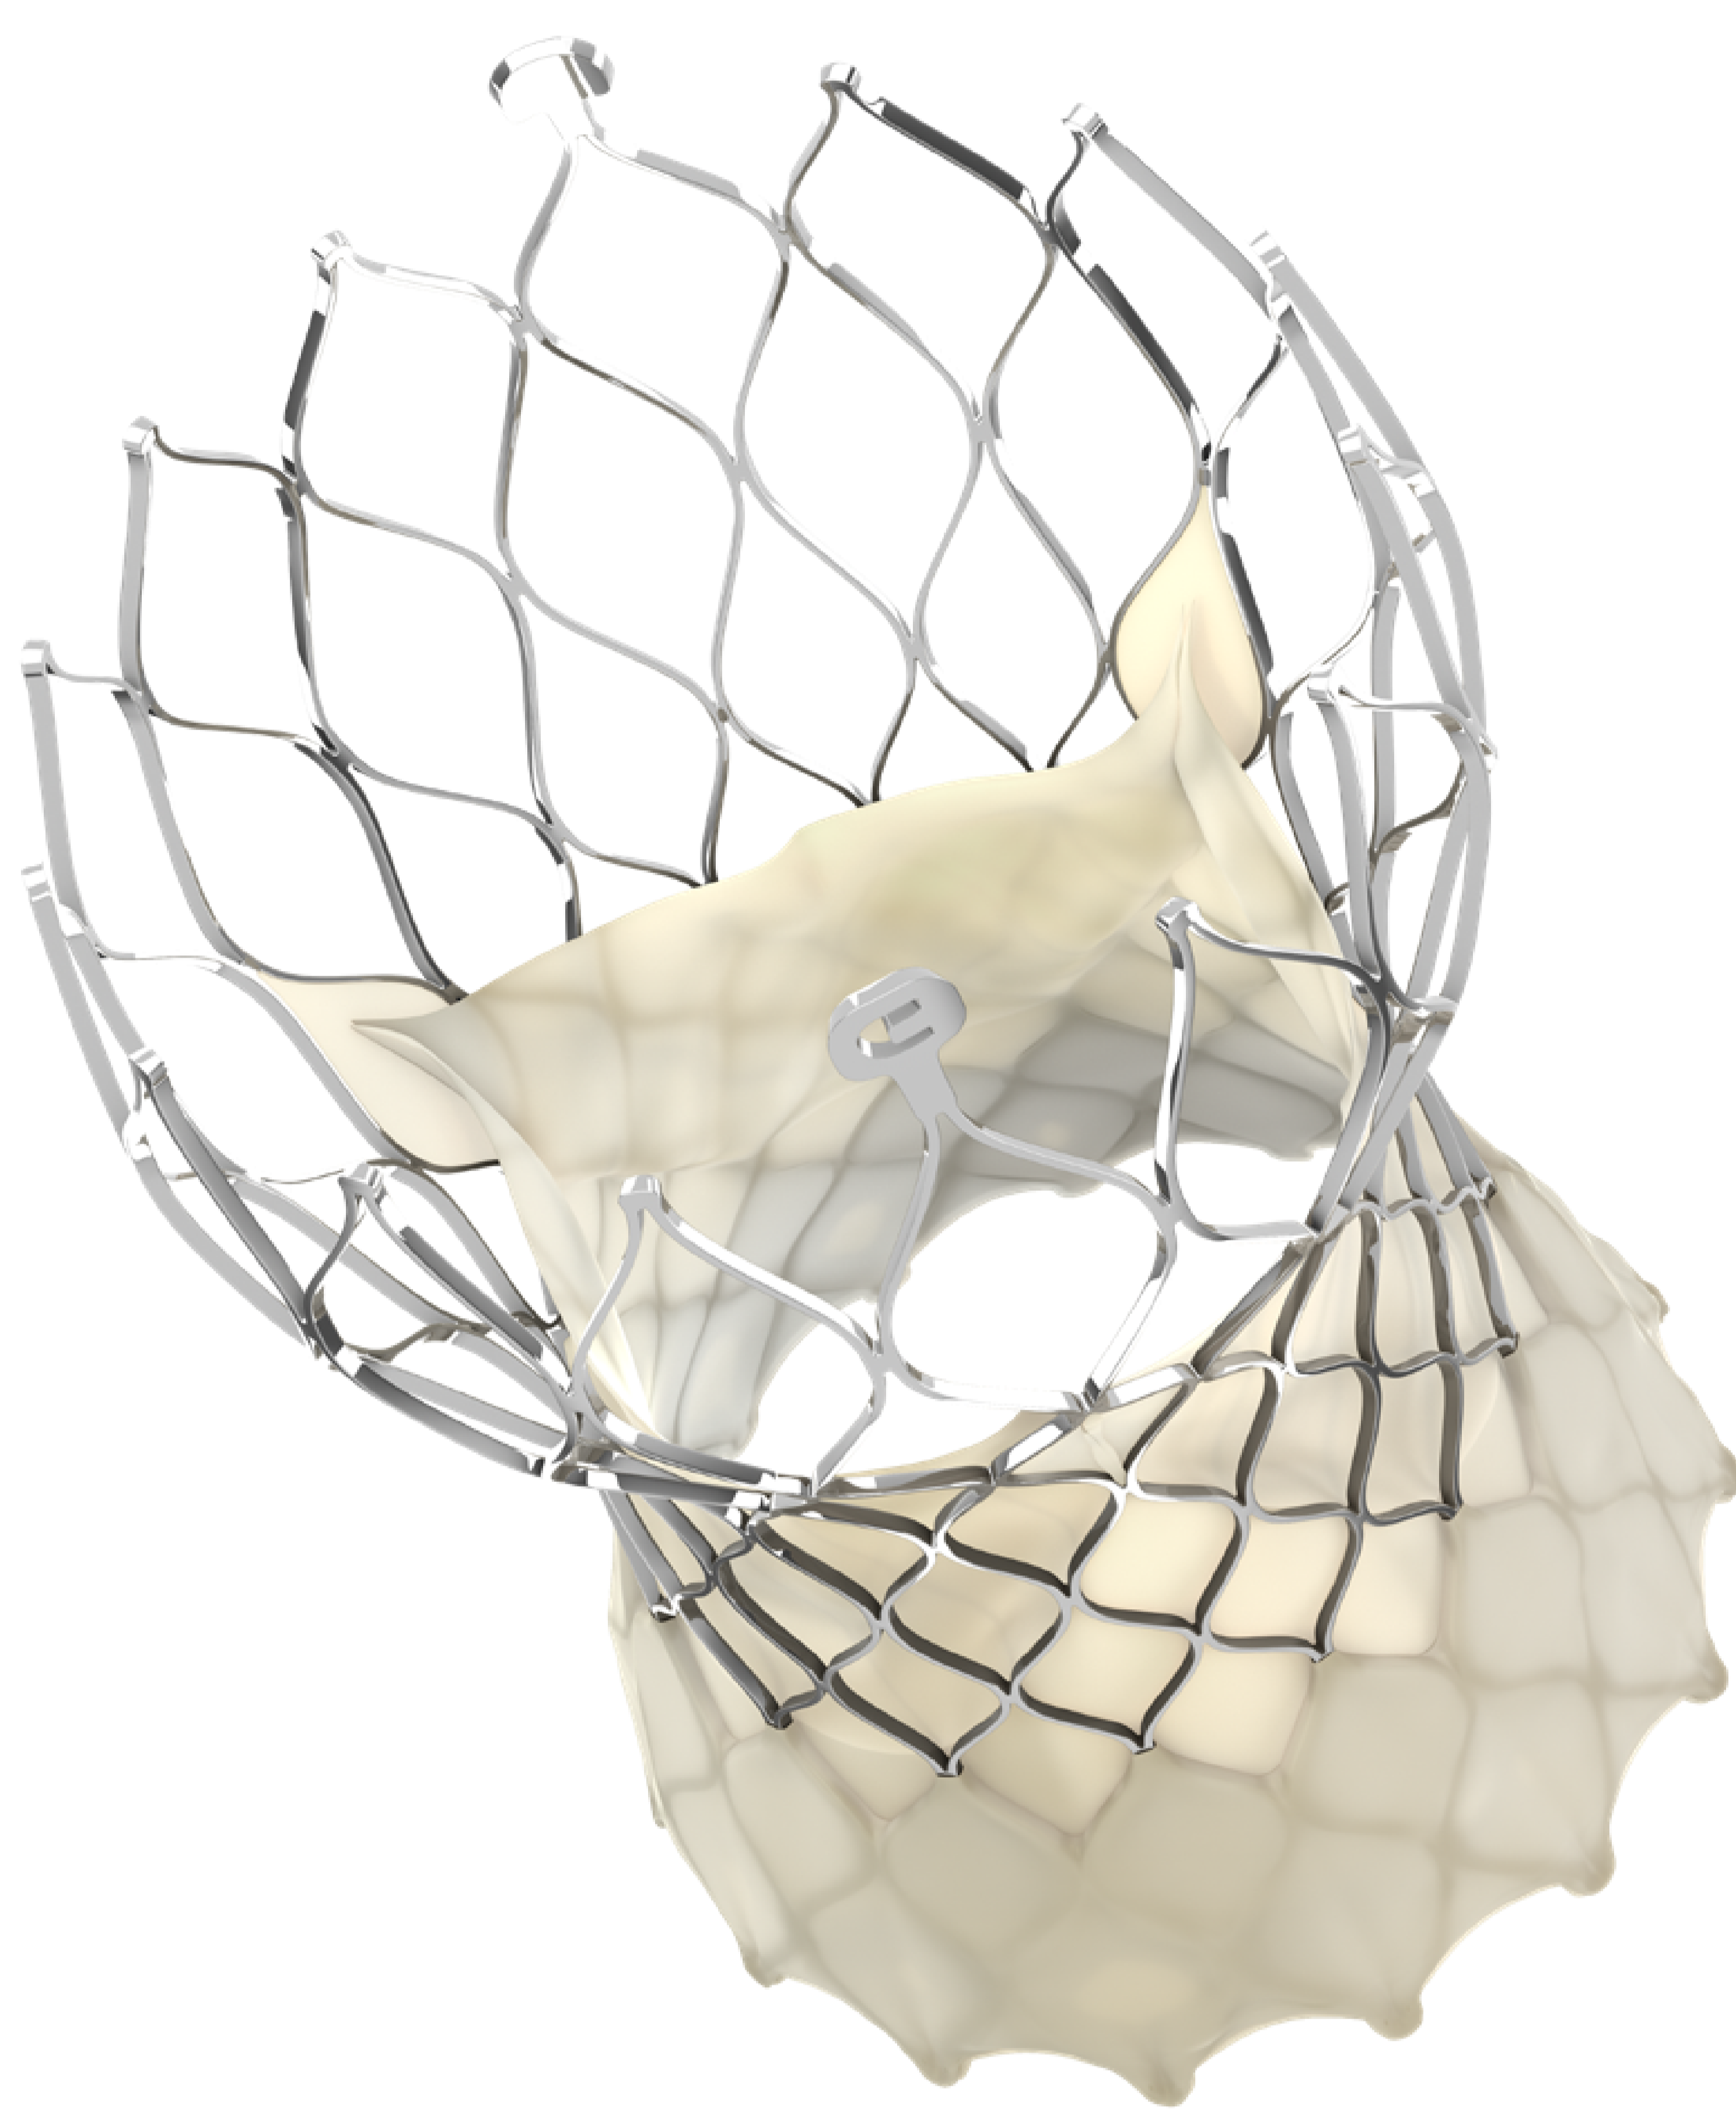


#### HEMODYNAMIC PERFORMANCE

for exceptional  
patient outcomes<sup>1</sup>

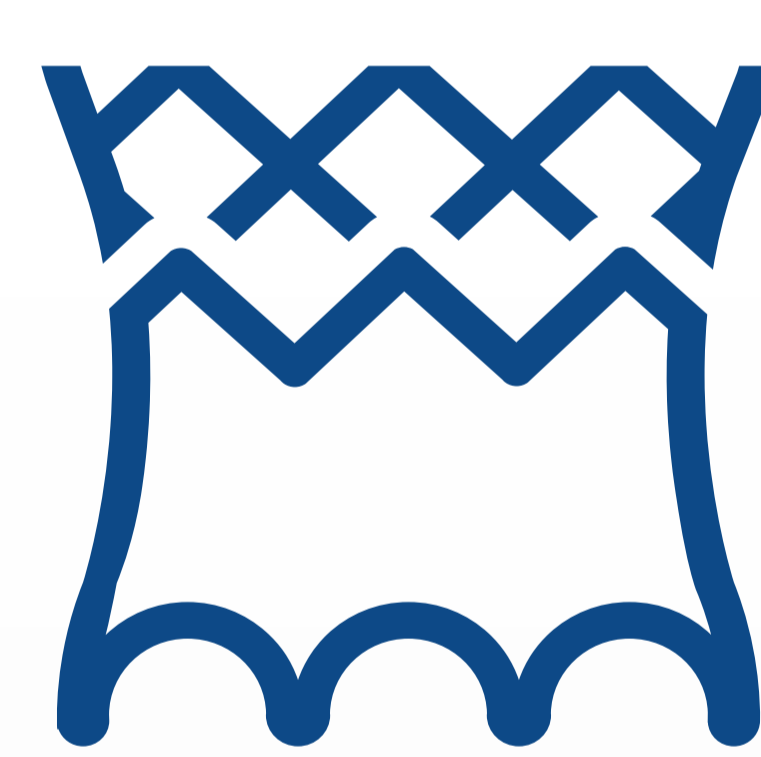

#### ADVANCED SEALING

for all valve sizes and  
across the broadest  
annular range<sup>†</sup>

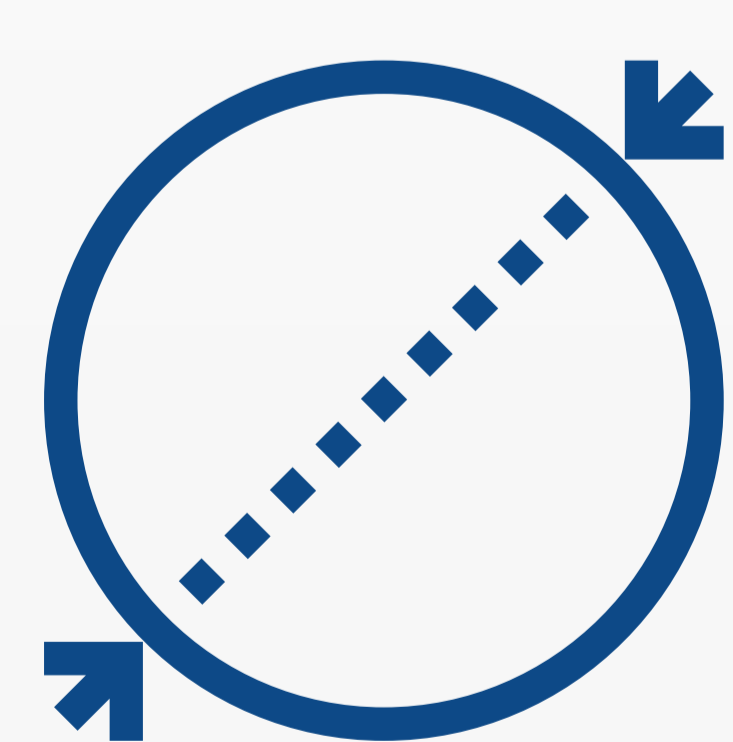

#### LOWEST DELIVERY PROFILE

for access down to 5.0 mm vessels  
with the 23-29 mm valves

1. Popma JJ, Deeb GM, Yakubov SJ, et al. Transcatheter Aortic-Valve Replacement with a Self-Expanding Valve in Low-Risk Patients. N Engl J Med. May 2, 2019;380(18):1706-1715.  
† Broadest annulus range based on CT derived diameters for self-expanding valves

See the CoreValve™ Evolut™ R, the CoreValve™ Evolut™ PRO and the Evolut™ PRO+ device manuals for detailed information regarding the instructions for use, the implant procedure, indications, contraindications, warnings, precautions, and potential adverse events. For further information, contact your local Medtronic representative and/or consult the Medtronic website at medtronic.eu.  
For applicable products, consult instructions for use on manuals.medtronic.com. Manuals can be viewed using a current version of any major internet browser. For best results, use Adobe Acrobat® Reader with the browser.  
The commercial name of the Evolut™ R device is Medtronic CoreValve™ Evolut™ R System, the commercial name of the Evolut™ PRO device is Medtronic CoreValve™ Evolut™ PRO System, and the commercial name of the Evolut™ PRO+ device is Medtronic Evolut™ PRO+ System.